


VERTICALE[®] MIS

VI-4120

[VI-4120.1; VI-4120.2; VI-4120.3]



D30003

1/3

D30104.b.YY
07.04.2022

D30049

Silony Medical GmbH
Leinfelder Straße 60
70771 Leinfelden-Echterdingen
Tel +49 711 78 25 25 0
Fax +49 711 78 25 25 11
www.silony-medical.com

labeling.silony-medical.com/contact


CE

MADE IN GERMANY

VERTICALE[®] MIS

VI-4120


[VI-4120.1; VI-4120.2; VI-4120.3]



D)



E)

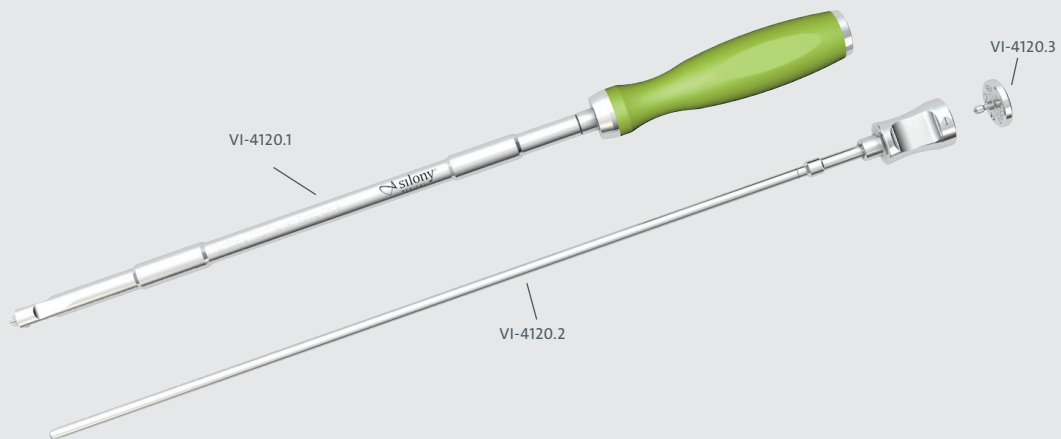

D30003

2/3

D30104.b.YY
07.04.2022

D30049

Silony Medical GmbH
Leinfelder Straße 60
70771 Leinfelden-Echterdingen
Tel +49 711 78 25 25 0
Fax +49 711 78 25 25 11
www.silony-medical.com

labeling.silony-medical.com/contact

CE

MADE IN GERMANY

VERTICALE[®] MIS

VI-4120

[VI-4120.1; VI-4120.2; VI-4120.3]




F)



G)



H)

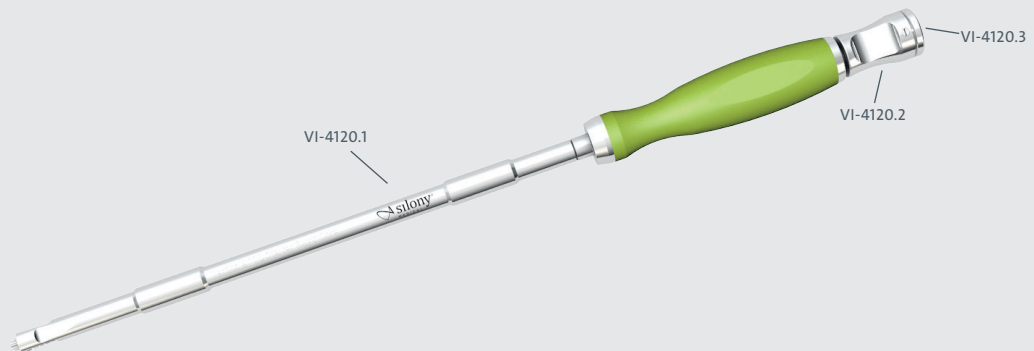

D30003

3/3

D30104.b.YY
07.04.2022

D30049

Silony Medical GmbH
Leinfelder Straße 60
70771 Leinfelden-Echterdingen
Tel +49 711 78 25 25 0
Fax +49 711 78 25 25 11
www.silony-medical.com

labeling.silony-medical.com/contact

CE

MADE IN GERMANY