


# VERTICALE<sup>®</sup> MIS




VI-4026

[ VI-1060; VI-1070; VI-4022; VI-4023; VI-4024; VI-4026 ]

A)

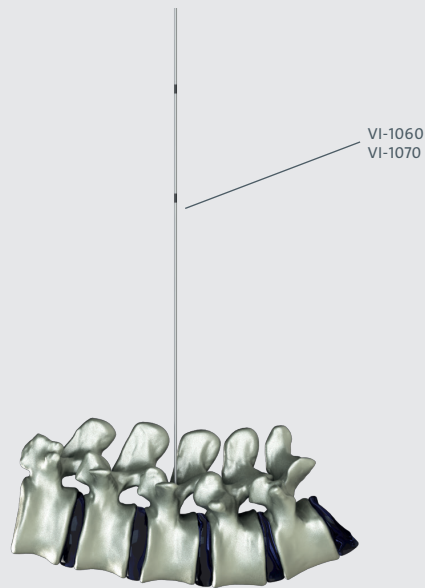

B)

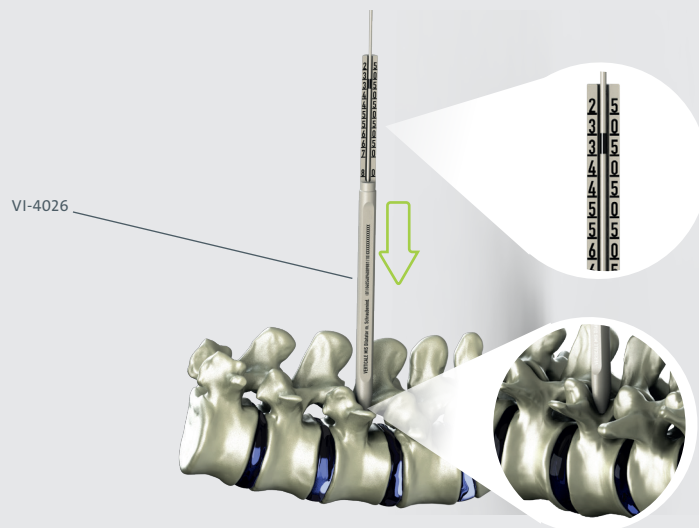

D30003

1/2

D30264.a.YY  
30.04.2021

D30049

Silony Medical GmbH

Leinfelder Straße 60  
70771 Leinfelden-Echterdingen, Germany

Tel +49 711 78 25 25 0

Fax +49 711 78 25 25 11

[www.silony-medical.com](http://www.silony-medical.com)

[elabeling.silony-medical.com/contact](https://www.silony-medical.com/contact)

MADE IN GERMANY


# VERTICALE® MIS




VI-4026

[ VI-1060; VI-1070; VI-4022; VI-4023; VI-4024; VI-4026 ]

C)

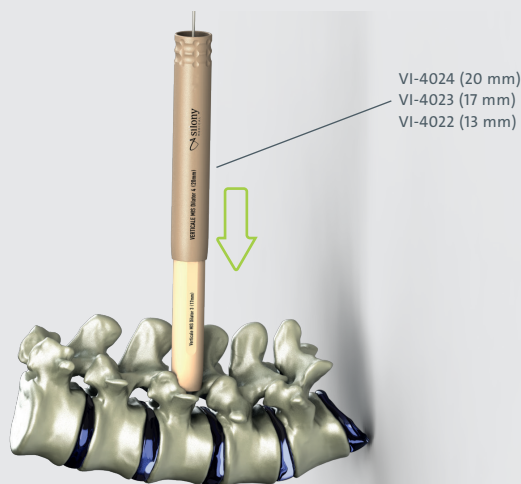

D)

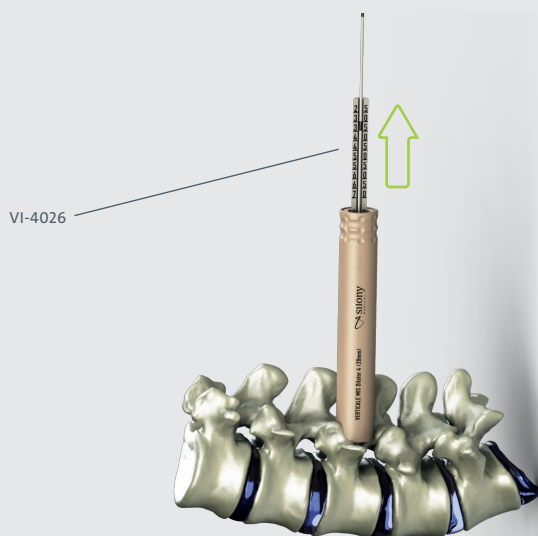

D30003

2/2

D30264.a.YY  
30.04.2021

D30049

Silony Medical GmbH

Leinfelder Straße 60

70771 Leinfelden-Echterdingen, Germany

Tel +49 711 78 25 25 0

Fax +49 711 78 25 25 11

[www.silony-medical.com](http://www.silony-medical.com)

[elabeling.silony-medical.com/contact](mailto:elabeling.silony-medical.com/contact)

MADE IN GERMANY