

**Instruction for Use (IFU046)****Implants of the STALIF L® portfolio****STALIF L.**  
**STALIF L. FLX****Important Information – please read before use!****Table of Contents**

1	Device Description.....	2
2	Indications for use .....	2
3	Contraindications .....	2
4	Warnings and precautions .....	2
5	Potential adverse events.....	3
6	Packaging, sterility and storage.....	4
8	Magnetic Resonance Imaging (MRI) Safety Information .....	5
9	Labeling and Symbols.....	5

This Instruction for use covers cages of the STALIF L and STALIF L FLX systems.

Other sets of manufacturer's instructions are available containing information required for application of the systems:

- Reprocessing Instructions for Instruments (LBL379)
- Surgical Technique Guide (STG019)

The system-specific product information can also be viewed at the following links:

- <https://elabeling.silony-medical.com>
- [www.silony-spine.com](http://www.silony-spine.com)

Any manufacturer liability is excluded in the event of non-compliance with the manufacturer's product information.

Prior to using a product distributed by Silony Spine, the surgeon is expected to carefully study the following indications/contraindications, recommendations, warnings, and advice as well as the product specific information. Silony Spine also recommends participation in appropriate user training.

Users and/or patients are required to report any (serious) incidents related to the device to the manufacturer and to the state competent authority.

Caution: Federal Law (USA) restricts these devices to sale by or on the order of a physician.

## 1 Device Description

### 1.1 General Information

The STALIF L Portfolio consists of lumbar intervertebral body fusion devices that are fixed to the superior and inferior vertebral bodies with cancellous lag bone screws augmented with an Anti- Back Out (ABO®) system.

The graft containment cavity is filled with bone graft (allograft and/or autograft) material. The STALIF L portfolio is available in two material options: PEEK (polyetheretherketone) and FLX (3D-printed osteoconductive porous titanium trabecular scaffold; FLX devices feature a combination of solid and porous, radiolucent FUSE-THRU titanium sections for reduced mechanical stiffness and improved visibility compared to solid titanium implants).

The STALIF L Integrated Interbody™ Fusion Cages consist of varying heights, widths, lengths, and lordotic angles to accommodate individual pathology and anatomical conditions.

STALIF L screws are to be used in conjunction with the STALIF L and STALIF L FLX cages. They are 4.5mm or 5.5mm outside diameter cancellous, self-tapping self-drilling type screws, augmented with an Anti Back-Out (ABO) system that are offered in a variety of lengths.

STALIF L Portfolio devices are Integrated Interbody fusion devices and are required to be used with supplementary fixation systems (e.g., pedicle screws) that have been cleared for use in the lumbar spine.

### 1.2 Material

STALIF L is manufactured from polyetheretherketone (PEEK) in accordance with ASTM F2026. X-ray marker rods/spheres are manufactured from unalloyed tantalum (Ta) per ASTM F560. STALIF L FLX is manufactured from printed titanium alloy (Ti6Al4V) in accordance with ASTM F3001.

STALIF L screws are manufactured from titanium alloy (Ti-6Al-4V) in accordance with ASTM F136 and ISO 5832- 3.

## 2 Indications for use

The STALIF L is indicated for use with autogenous bone graft in patients with degenerative disc disease (DDD) at one or two contiguous levels from L2 to L5. The STALIF L FLX is indicated for use with bone graft (autograft bone and/or allogenic bone graft composed of cancellous and/or corticocancellous bone graft) in patients with degenerative disc disease (DDD) at one or two contiguous levels from L2 to L5. These DDD patients may also have up to Grade I spondylolisthesis or retrolisthesis at the involved levels. DDD is defined as discogenic back pain with degeneration of the disc confirmed by history and radiographic studies. These patients should be skeletally mature and have had six months of non-operative treatment. Patients with previous non-fusion spinal surgery at the treated level may be treated. These implants may be implanted via a laparoscopic or an open lateral approach.

The STALIF L/STALIF L FLX is required to be used with supplementary fixation systems (e.g., pedicle screws) that have been cleared for use in the lumbar spine.

## 3 Contraindications

- Osteoporosis, sepsis
- Infection or inflammation at or near the operative site
- Fever of undetermined origin
- Allergy to implant materials
- Patient is unable or unwilling to follow post-operative instructions
- Disease or condition which precludes the possibility of healing
- Prior fusion at the level to be treated
- Any conditions not described in the indications

## 4 Warnings and precautions

- Patients with previous spinal surgery at the levels to be treated may not experience the same clinical outcomes as those without a previous surgery.

- Selection of an appropriately sized device for the patient is important and increases the likelihood of a satisfactory outcome.
- The implantation of the intervertebral body fusion device should be performed only by experienced spinal surgeons with specific training in the use of this type of device.
- Do not use if the package is damaged or opened. Contents may not be sterile.
- Do not use if current date exceeds label expiry date.
- Do not re-sterilize sterile implants.
- Instrumentation provided with the implants must be used in accordance with the approved surgical technique.
- Do not use excessive force when introducing and positioning the implant within the intervertebral body space to avoid damaging the implant.
- Re-usable surgical instruments must be decontaminated and sterilized prior to next use.
- Do not reuse the device even if the device shows no external signs of damage. Internal stresses from previous use may cause early failure.
- Do not intermix implants of different metallic alloy types in the same construct. Premature device failure and/or infection in the patient may occur.
- On insertion of the screw into the STALIF L/ STALIF L FLX device, ensure soft tissue is not trapped between the head of the screw and the device.
- STALIF L screws must be used in accordance with Table 1, to ensure minimum depth of screw in bone is greater than 12mm.
- Use caution when using STALIF L/ STALIF L FLX devices at contiguous levels to avoid screw interaction between adjacent level STALIF L screws, particularly when using the longer length screws (30mm - 40mm) with the smaller height cages (8mm - 12mm) see table 1.
- When using the STALIF L/ STALIF L FLX system, the physician/surgeon should consider the height of the patient vertebral bodies in the selection of STALIF L screw lengths, particularly in contiguous level use.

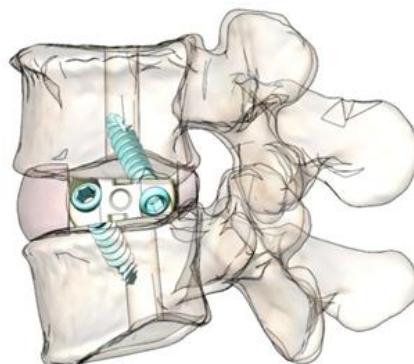


Figure 1. STALIF L

Table 1: Restrictions on screw length according to cage height

STALIF L Screw dimension	Restrictions on use according to cage height
Ø4.5mm (All lengths)	STALIF L: Use with <b>8mm and 10mm height</b> cages only STALIF L FLX: <b>DO NOT USE</b>
Ø5.5mm x 25mm	STALIF L: Use with <b>12mm and 14mm height</b> cages only STALIF L FLX: Use with <b>8mm-14mm height</b> cages only
Ø5.5mm x 30, 35, 40mm	STALIF L: Use with <b>12mm and taller height</b> cages only STALIF L FLX: Use with <b>8mm and taller height</b> cages only

## 5 Potential adverse events

Potential risks or adverse effects identified with the use of this intervertebral body fusion device, which may require additional surgery are similar to those of other spinal systems, and include, but are not limited to:

- Early or late loosening of the components
- Bending or breakage of the components
- Foreign body (allergic) reaction
- Infection
- Pseudoarthrosis (i.e., non-union)
- Bone loss due to resorption or stress shielding
- Loss of neurological function
- Neurological difficulties such as radiculopathy, paresthesia, new or continued pain, numbness/tingling, neuroma, dural tears, neuropathy and neurologic deficit
- Loss or impairment of bowel, sexual, and/or bladder function
- Vascular damage resulting in excessive blood loss
- Bone graft complications including pain, fracture or wound healing problems
- Spinal cord impingement or damage
- Fracture, damage, degenerative changes or instability of any bone above and/or below the level of surgery
- Additional surgery
- Rarely, some complications may be fatal

## 6 Packaging, sterility and storage

### 6.1 Packaging

- Packaging of the components should be intact upon receipt. Damaged packages or products should not be used and should be returned to Silony Spine.

### 6.2 Storage

- The STALIF L/ STALIF L FLX device can be shipped and stored at ambient conditions.

### 6.3 Sterility

- All components of the STALIF L/ STALIF L FLX device are provided sterile by gamma irradiation for single use only.
- System instrumentation must be sterilized per AAMI ST79 as indicated in instruction for use for cleaning and sterilization (LBL379).

## 7 Notes for application

Use of the STALIF L/ STALIF L FLX device should only be considered when the following pre-operative, intra-operative and post-operative conditions exist:

### 7.1 Pre-operative

- Patient meets the indication criteria described and does not have any contraindications.
- The surgeon should determine the construct prior to surgery to ensure that the required components in the necessary sizes are available.

### 7.2 Intra-operative

- The surgeon follows the surgical technique and instructions for use of the device.
- All components are inspected and determined to be free of damage..
- Bone graft (autograft and/or allograft) is placed in the area to be fused.

### 7.3 Post-operative

- The choice to administer post-operative antibiotics is at the discretion of the surgeon.
- Post-operative mobilization and rehabilitation is at the discretion of the surgeon dependent on clinical and radiological progress.
- The need for external orthotic support is not mandatory with the final choice based on surgeon preference, patient condition and intra-operative findings that might influence implant security.
- The patient is to be instructed to reduce undue stress on the implant as a precaution to avoid clinical problems that could result in fixation failure.
- The patient is to be instructed to follow the post-operative regime.

## 8 Magnetic Resonance Imaging (MRI) Safety Information

- Non-clinical testing demonstrated that the STALIF L/ STALIF L FLX is MR Conditional. A patient with this device can be scanned safely in an MR system under the following conditions:
  - Static magnetic field of 1.5 Tesla and 3 Tesla only.
  - Maximum spatial gradient magnetic field of 2,000 Gauss/cm (20 T/m)
  - Maximum MR System reported whole body averaged specific absorption rate (SAR) of 2 W/kg for 15 minutes of scanning (i.e., per pulse sequence) in the Normal Operating Mode.
- Under the scan conditions defined, the STALIF L/ STALIF L FLX implant is expected to produce a maximum temperature rise of 2.0°C after 15 minutes of continuous scanning.
- In non-clinical testing, the image artifacts caused by the STALIF L/ STALIF L FLX implant extends approximately 10mm from this implant when imaged using gradient echo pulse sequence and a 3Tesla MR system.

## 9 Labeling and Symbols

Symbols according to ISO 15223-1 and 21 CFR 801 Labeling.

Symbol	Explanatory Text
	Manufacturer
	Date of manufacture <i>Including the date in the following format: YYYY-MM-DD</i>
	Article number
	Lot number
	Number of items
	Medical device
	Unique device identification
	Use by date <i>Including the year and month in the following format: YYYY-MM-DD</i>
	Consult instruction for use
	WWW.SILONYSPINE.COM
	Caution
	Sterilized using irradiation
	Do not reuse
	Do not resterilize
	Do not use if the packaging is damaged
	Keep dry
	Keep away from sunlight
	MR* conditional (The term MR is synonymous with MRI and means magnetic resonance imaging.)
	Metal detectors can trigger alarm due to the implant
	Patient Identification

	Health care centre or doctor
	Date (of implantation)
	Contact
	Silony Logo (for identification of the legal manufacturer in the course of direct marking of products)



Silony Medical GmbH  
Leinfelder Straße 60  
70771 Leinfelden-Echterdingen  
Germany

Telephone: +49 (0)711-782 525 0  
Fax: +49 (0)711-782 525 11  
E-Mail: [info.stuttgart@silony-medical.com](mailto:info.stuttgart@silony-medical.com)



<https://www.silony spine.com/contact>



[www.silony-medical.com/ifu](http://www.silony-medical.com/ifu)