

VERTICALE[®] MIS

VI-4180




GI-1TRK
Ratchet T-Handle cannulated



VI-4180
VERTICALE MIS Working Tower
Removal Tool



To disengage the working towers, the VERTICALE MIS Working Tower Removal Tool must be connected with the handle and then inserted into the MIS Working Tower. The working tower is disengaged from the pedicle screw head by turning anti-clockwise with slight downward pressure. The working tower is only fully disengaged from the screw and can be removed when the yellow marking on the working tower becomes visible (inset). In doing so, the VERTICALE MIS Counter Torque can be used to stabilise the rotation when disengaging the MIS Working Towers.

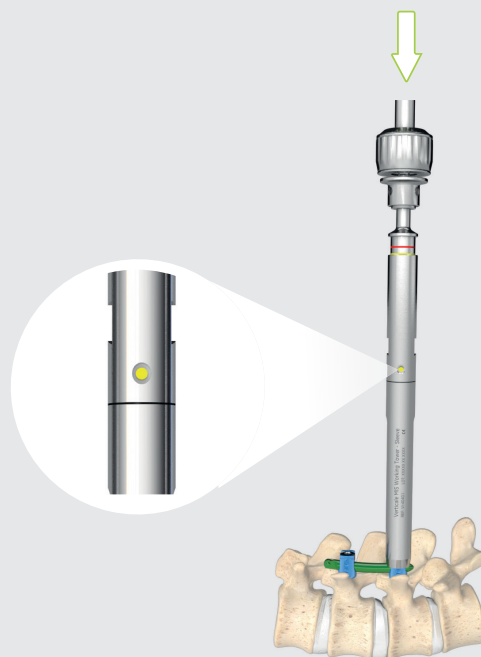

Removal of the VERTICALE MIS Working Towers using the VERTICALE MIS Working Tower Removal Tool

D60007

D60005

D60037.a.EN
30.11.2018

Silony Medical Corp.

8200 NW 27th Street, Suite 104
Doral, FL 33122, USA
Phone +1 305 916 0016



www.silony-medical.com

Silony Medical GmbH

Leinfelder Straße 60
70771 Leinfelden-Echterdingen, Germany
Phone +49 711 78 25 25 0
Fax +49 711 78 25 25 11

MADE IN GERMANY